

COSMETIC BRACKETS

The powerful combination of clinical performance and aesthetic appeal has resulted in unprecedented demand for cosmetic brackets. Desired by patients and admired by doctors, ODP's line of ceramic and composite bracket systems gives your patients the allure they deserve, while providing you with a quality, affordable alternative to traditional metal brackets. Choose from our innovative line of Lucent™ and Prism™ composite brackets, or our trendy Mirage™, Clarion™ and Diamante™ ceramic bracket systems. Either way, your patients will love the way they look both during and after treatment.

Beautifully Functional


ODP's attractive, comfortable Lucent™ composite brackets feature a nickel-free silver alloy-lined archwire slot that makes them a safe alternative for nickel-sensitive patients. The metal liner is precisely integrated into the bracket body, creating a pleasantly aesthetic device that delivers the sliding mechanics of a metal slot.



Powerfully Flexible

The special composite formulation from which the appliance is manufactured produces a bracket that exhibits a high tensile strength. The result is a strong polyurethane bracket with superior sliding mechanics that are equal to or greater than stainless steel brackets.

Available in Roth, MBT, and Standard Edgewise prescriptions, Lucent™ composite brackets offer the pleasing aesthetics and comfort desired by patients, along with the clinical functionality demanded by doctors.

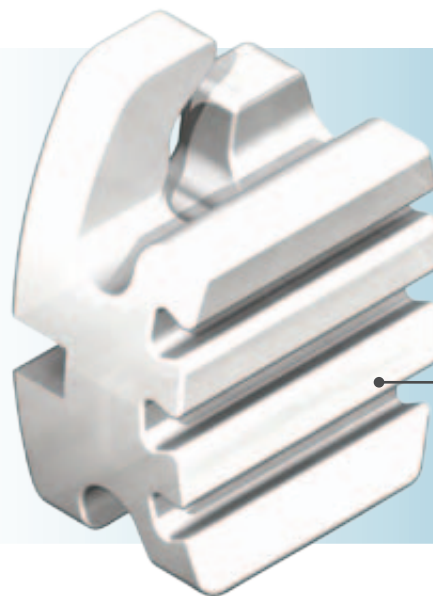

A Strong Mechanical Bond. Every Time.

ODP's Lucent™ brackets feature a distinctively designed mushroom grooved base for increased surface contact, allowing for excellent adhesion.



The brackets are designed with a porous coating that provides millions of additional undercuts that firmly grip the adhesive. As a result, additional primer agents are not required to bond Lucent™ brackets to the tooth's enamel.

Lucent™ brackets feature superior retention and easy debonding characteristics.

Lucent™

METAL-LINED COMPOSITE BRACKET SYSTEM

by Orthodontic Design and Production, Inc.

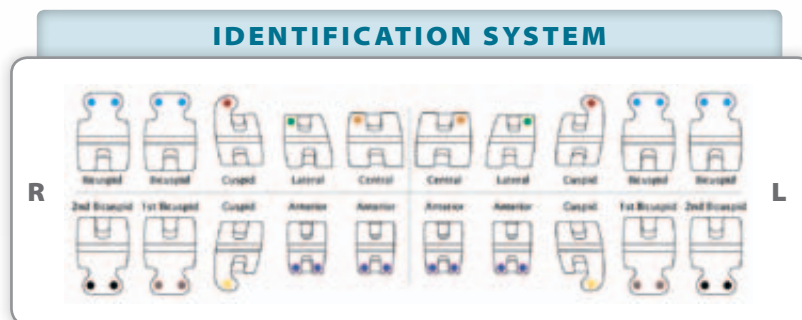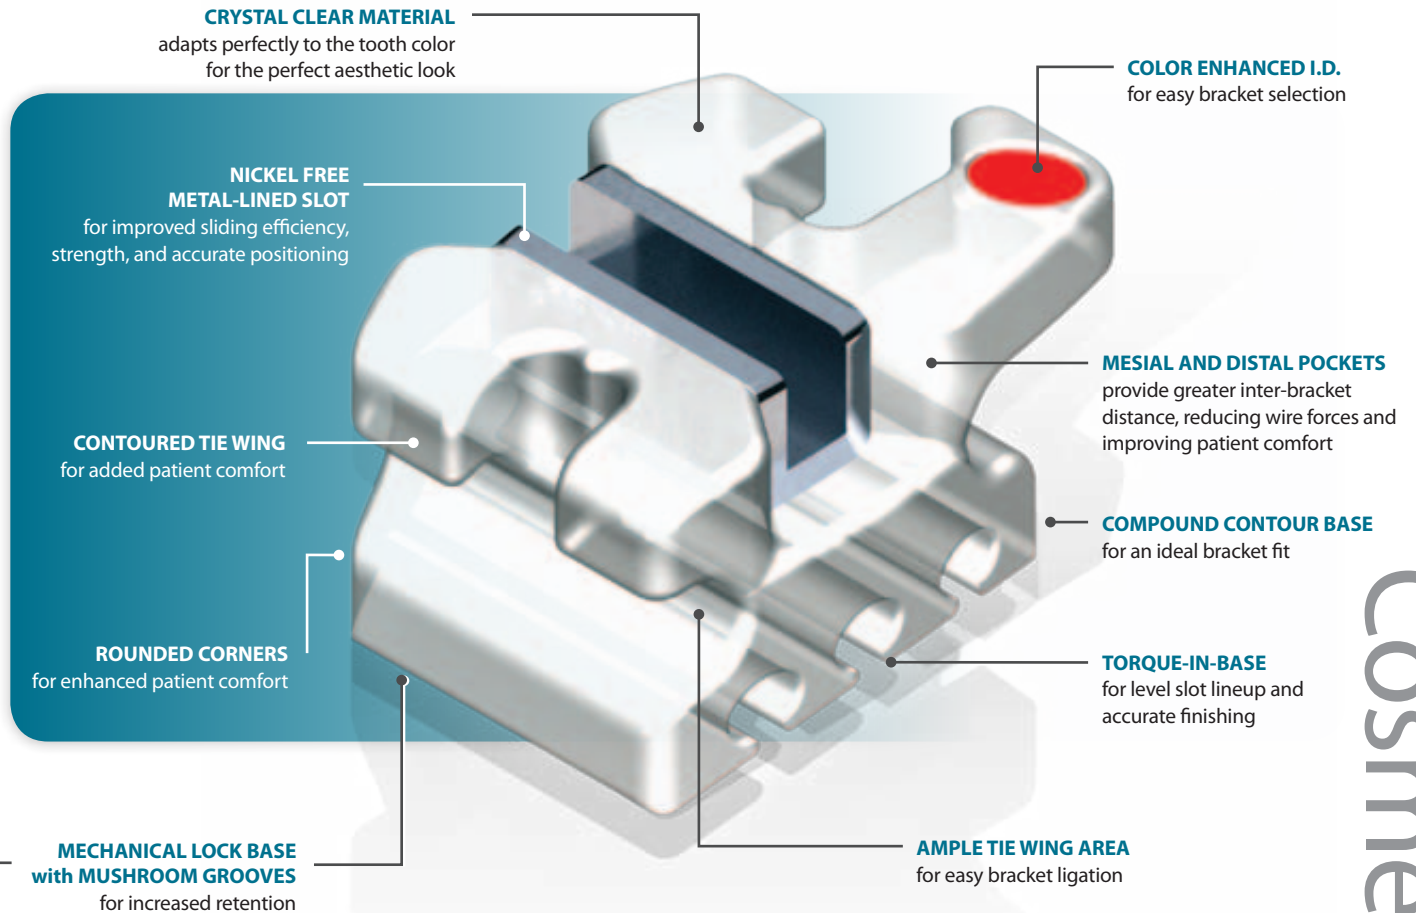

Cosmetic Brackets

LUCENT™ METAL-LINED COMPOSITE BRACKET SYSTEM

Roth[†] Prescription

Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	+12°	+5°	0°	3.9 mm	R	●	40-U1-8R	40-U1-2R
					L	●	40-U1-8L	40-U1-2L
Lateral	+8°	+9°	0°	3.3 mm	R	●	40-U2-8R	40-U2-2R
					L	●	40-U2-8L	40-U2-2L
Cuspid	0°	+11°	+4°	3.3 mm	R	●	40-U3-8R	40-U3-2R
					L	●	40-U3-8L	40-U3-2L
Cuspid Hk					R	●	40-U3-8RK	40-U3-2RK
					L	●	40-U3-8LK	40-U3-2LK
1 st & 2 nd Bicuspid	-7°	0°	0°	3.3 mm	U	●●	40-U4-8U	40-U4-2U
1 st & 2 nd Bicuspid Hk					U	●●	40-U4-8UK	40-U4-2UK

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	0°	0°	0°	2.8 mm	U	●●	40-L1-8U	40-L1-2U
Cuspid	-11°	+5°	+2°	3.3 mm	R	●	40-L3-8R	40-L3-2R
					L	●	40-L3-8L	40-L3-2L
Cuspid Hk					R	●	40-L3-8RK	40-L3-2RK
					L	●	40-L3-8LK	40-L3-2LK
1 st Bicuspid	-17°	0°	0°	3.3 mm	U	●●	40-L4-8U	40-L4-2U
1 st Bicuspid Hk					U	●●	40-L4-8UK	40-L4-2UK
2 nd Bicuspid	-22°	0°	0°	3.3 mm	U	●●	40-L5-8U	40-L5-2U
2 nd Bicuspid Hk					U	●●	40-L5-8UK	40-L5-2UK

Full Sets	.018	.022
Upper/Lower 5X5 No Hooks	40K-NHK-18	40K-NHK-22
Upper/Lower 5X5 No Hook on 3	40K-3-18	40K-3-22
Upper/Lower 5X5 No Hooks on 3, 4, & 5	40K-345-18	40K-345-22

Edgewise Prescription

Maxillary & Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	0°	0°	0°	3.9 mm	U	---	42-CENT-18	42-CENT-22
Lateral	0°	0°	0°	3.3 mm	U	---	42-LAT-18	42-LAT-22
Cuspid	0°	0°	0°	3.3 mm	U	---	42-CUSP-18	42-CUSP-22
Bicuspid	0°	0°	0°	3.3 mm	U	---	42-BIC-18	42-BIC-22
Lower Anterior	0°	0°	0°	2.8 mm	U	---	42-ANT-18	42-ANT-22

Full Sets	.018	.022
Upper/Lower 5X5 No Hooks	42K-EDGE-18	42K-EDGE-22

Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

[†] ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

LUCENT™ METAL-LINED COMPOSITE BRACKET SYSTEM

MBT[†] Prescription

Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	+17°	+4°	0°	3.9 mm	R	●	41-U1-8R	41-U1-2R
					L	●	41-U1-8L	41-U1-2L
Lateral	+10°	+8°	0°	3.3 mm	R	●	41-U2-8R	41-U2-2R
					L	●	41-U2-8L	41-U2-2L
Cuspid	-7°	+8°	0°	3.3 mm	R	●	41-U3-8R	41-U3-2R
					L	●	41-U3-8L	41-U3-2L
Cuspid Hk	0°	+8°	0°	3.3 mm	R	●	41-U3-8RK	41-U3-2RK
					L	●	41-U3-8LK	41-U3-2LK
1 st & 2 nd Bicuspid	-7°	0°	0°	3.3 mm	U	●●	41-U4-8U	41-U4-2U
1 st & 2 nd Bicuspid Hk					U	●●	41-U4-8UK	41-U4-2UK

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	-6°	0°	0°	2.8 mm	U	●●	41-L1-8U	41-L1-2U
Cuspid	-6°	+3°	0°	3.3 mm	R	●	41-L3-8R	41-L3-2R
					L	●	41-L3-8L	41-L3-2L
Cuspid Hk	0°	+3°	0°	3.3 mm	R	●	41-L3-8RK	41-L3-2RK
					L	●	41-L3-8LK	41-L3-2LK
1 st Bicuspid	-12°	+2°	0°	3.3 mm	R	●	41-L4-8R	41-L4-2R
					L	●	41-L4-8L	41-L4-2L
1 st Bicuspid Hk					R	●	41-L4-8RK	41-L4-2RK
					L	●	41-L4-8LK	41-L4-2LK
2 nd Bicuspid	-17°	+2°	0°	3.3 mm	R	●	41-L5-8R	41-L5-2R
					L	●	41-L5-8L	41-L5-2L
2 nd Bicuspid Hk					R	●	41-L5-8RK	41-L5-2RK
					L	●	41-L5-8LK	41-L5-2LK

Full Sets	.018	.022
Upper/Lower 5x5 No Hooks	41K-NHK-18	41K-NHK-22
Upper/Lower 5x5 Hook on 3	41K-3-18	41K-3-22
Upper/Lower 5x5 Hooks on 3, 4, & 5	41K-345-18	41K-345-22



Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

[†] ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

Cuspids with 0° torque come standard in kits. Please specify when ordering if you require alternate torque.

Cosmetic Brackets


The Preferred Aesthetic Choice

Your patients will be thrilled with the transparent aesthetic appearance of Prism™ composite brackets. Not only are Prism™ composite brackets nearly invisible, but the special composite formulation from which they are manufactured produces a bracket that displays a high tensile strength. The result is a strong polyurethane bracket with superior sliding mechanics that are equal to or greater than stainless steel brackets.



Proven Clinical Performance

Available in Roth, MBT, and Standard Edgewise prescriptions, Prism™ composite brackets offer the pleasing aesthetics and comfort desired by patients, along with the clinical functionality demanded by doctors. Prism's™ exceptionally high translucency provides superb aesthetics - a marketable advantage that appeals to patients of all ages. With ODP's Prism™ brackets, patients experience a more comfortable, attractive treatment experience, while doctors achieve the results they desire.

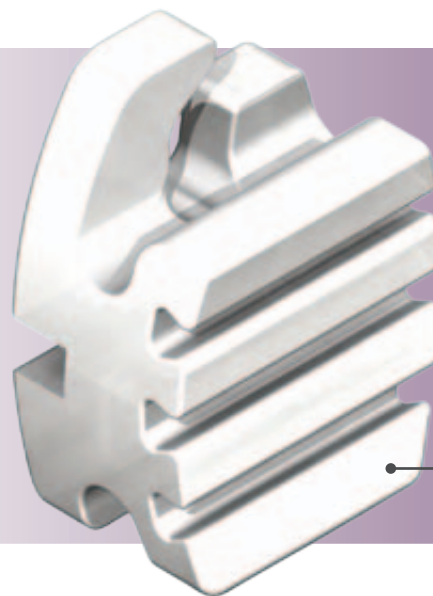

Innovation, from the Bottom Up

ODP's Prism™ brackets feature a distinctively designed dovetailed base for increased surface contact, allowing for excellent adhesion.



The brackets are designed with a porous coating that provides millions of additional undercuts that firmly grip the adhesive. As a result, additional primer agents are not required to bond Prism™ brackets to the tooth's enamel.

Prism™ brackets feature superior retention and easy debonding characteristics.



Prism™ COMPOSITE BRACKET SYSTEM

by Orthodontic Design
and Production, Inc.

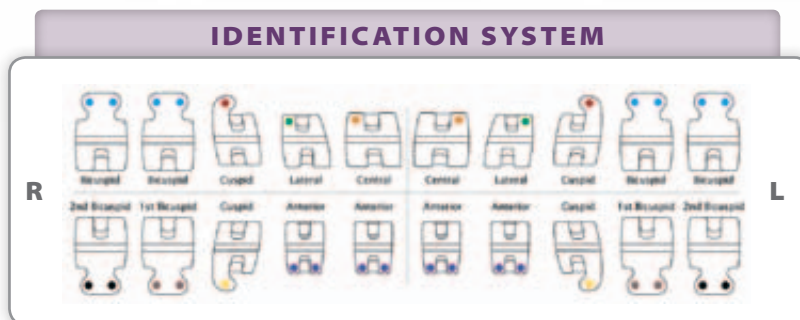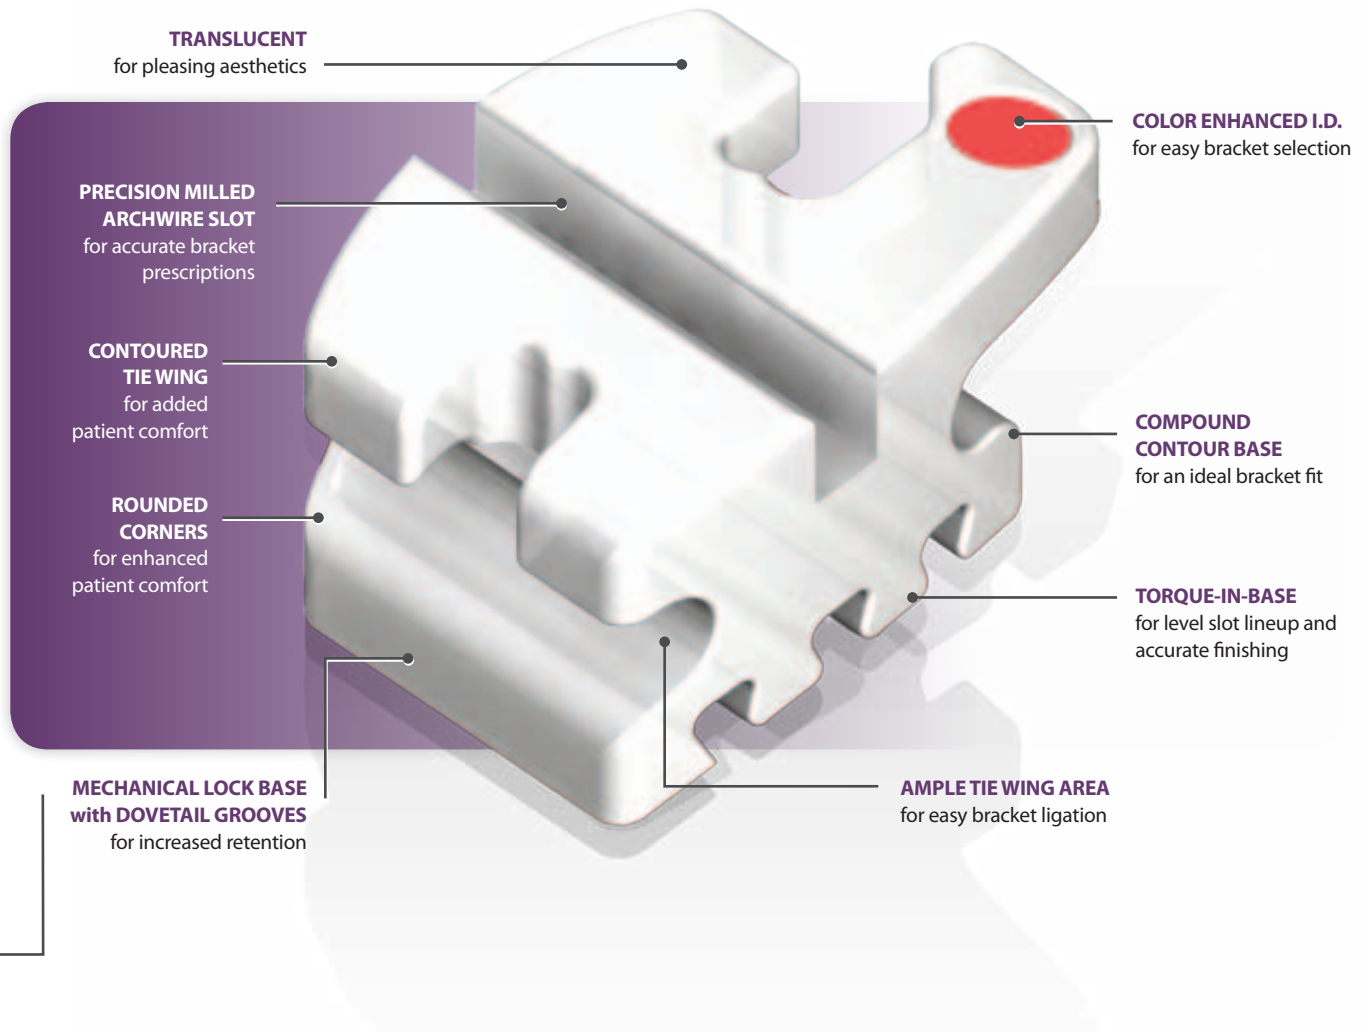

Cosmetic Brackets

PRISM™ COMPOSITE BRACKET SYSTEM

Roth[†] Prescription

Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	+12°	+5°	0°	3.9 mm	R	●	45-U1-8R	45-U1-2R
					L	●	45-U1-8L	45-U1-2L
Lateral	+8°	+9°	0°	3.3 mm	R	●	45-U2-8R	45-U2-2R
					L	●	45-U2-8L	45-U2-2L
Cuspid	0°	+11°	+4°	3.3 mm	R	●	45-U3-8R	45-U3-2R
					L	●	45-U3-8L	45-U3-2L
Cuspid Hk					R	●	45-U3-8RK	45-U3-2RK
					L	●	45-U3-8LK	45-U3-2LK
1 st & 2 nd Bicuspid	-7°	0°	0°	3.3 mm	U	●●	45-U4-8U	45-U4-2U
1 st & 2 nd Bicuspid Hk					U	●●	45-U4-8UK	45-U4-2UK

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	0°	0°	0°	2.8 mm	U	●●	45-L1-8U	45-L1-2U
Cuspid	-11°	+5°	+2°	3.3 mm	R	●	45-L3-8R	45-L3-2R
					L	●	45-L3-8L	45-L3-2L
Cuspid Hk					R	●	45-L3-8RK	45-L3-2RK
					L	●	45-L3-8LK	45-L3-2LK
1 st Bicuspid	-17°	0°	0°	3.3 mm	U	●●	45-L4-8U	45-L4-2U
1 st Bicuspid Hk					U	●●	45-L4-8UK	45-L4-2UK
2 nd Bicuspid	-22°	0°	0°	3.3 mm	U	●●	45-L5-8U	45-L5-2U
2 nd Bicuspid Hk					U	●●	45-L5-8UK	45-L5-2UK

Full Sets	.018	.022
Upper/Lower 5X5 No Hooks	45K-NHK-18	45K-NHK-22
Upper/Lower 5X5 No Hook on 3	45K-3-18	45K-3-22
Upper/Lower 5X5 No Hooks on 3, 4, & 5	45K-345-18	45K-345-22

Edgewise Prescription

Maxillary & Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	0°	0°	0°	3.9 mm	U	---	47-CENT-18	47-CENT-22
Lateral	0°	0°	0°	3.3 mm	U	---	47-LAT-18	47-LAT-22
Cuspid	0°	0°	0°	3.3 mm	U	---	47-CUSP-18	47-CUSP-22
Bicuspid	0°	0°	0°	3.3 mm	U	---	47-BIC-18	47-BIC-22
Lower Anterior	0°	0°	0°	2.8 mm	U	---	47-ANT-18	47-ANT-22

Full Sets	.018	.022
Upper/Lower 5x5 No Hooks	47K-EDGE-18	47K-EDGE-22

Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

[†] ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

PRISM™ COMPOSITE BRACKET SYSTEM
MBT[†] Prescription
Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	+17°	+4°	0°	3.9 mm	R	●	46-U1-8R	46-U1-2R
					L	●	46-U1-8L	46-U1-2L
Lateral	+10°	+8°	0°	3.3 mm	R	●	46-U2-8R	46-U2-2R
					L	●	46-U2-8L	46-U2-2L
Cuspid	-7°	+8°	0°	3.3 mm	R	●	46-U3-8R	46-U3-2R
					L	●	46-U3-8L	46-U3-2L
Cuspid Hk	0°	+8°	0°	3.3 mm	R	●	46-U3-8RK	46-U3-2RK
					L	●	46-U3-8LK	46-U3-2LK
1 st & 2 nd Bicuspid	-7°	0°	0°	3.3 mm	U	●●	46-U4-8U	46-U4-2U
1 st & 2 nd Bicuspid Hk					U	●●	46-U4-8UK	46-U4-2UK

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	-6°	0°	0°	2.8 mm	U	●●	46-L1-8U	46-L1-2U
Cuspid	-6°	+3°	0°	3.3 mm	R	●	46-L3-8R	46-L3-2R
					L	●	46-L3-8L	46-L3-2L
Cuspid Hk	0°	+3°	0°	3.3 mm	R	●	46-L3-8RK	46-L3-2RK
					L	●	46-L3-8LK	46-L3-2LK
1 st Bicuspid	-12°	+2°	0°	3.3 mm	R	●	46-L4-8R	46-L4-2R
					L	●	46-L4-8L	46-L4-2L
1 st Bicuspid Hk					R	●	46-L4-8RK	46-L4-2RK
					L	●	46-L4-8LK	46-L4-2LK
2 nd Bicuspid	-17°	+2°	0°	3.3 mm	R	●	46-L5-8R	46-L5-2R
					L	●	46-L5-8L	46-L5-2L
2 nd Bicuspid Hk					R	●	46-L5-8RK	46-L5-2RK
					L	●	46-L5-8LK	46-L5-2LK

Full Sets	.018	.022
Upper/Lower 5x5 No Hooks	46K-NHK-18	46K-NHK-22
Upper/Lower 5x5 Hook on 3	46K-3-18	46K-3-22
Upper/Lower 5x5 Hooks on 3, 4, & 5	46K-345-18	46K-345-22



Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

[†] ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

Cuspids with 0° torque come standard in kits. Please specify when ordering if you require alternate torque.

ORDER BY FAX: (760) 734-1735 OR E-MAIL: info@odpinc.com

Cosmetic Brackets

Mirage™ Ceramic Brackets... The Choice is Clear.

ODP's Mirage™ ceramic bracket system is the "clear choice" for aesthetically-minded patients. Small and smooth, with rounded corners that provide the ultimate in patient comfort, Mirage™ ceramic brackets are nearly invisible, blending inconspicuously into the oral cavity to give patients the confidence they need and the results they desire.


Composed of 99.9 percent pure polycrystalline alumina oxide, Mirage™ ceramic brackets are impervious to stains and discolorations, helping them stay transparent for the duration of the treatment to reveal nothing but a beautiful smile. Your patients will be thrilled with the fully transparent aesthetic appearance of Mirage™ ceramic brackets. It doesn't get any clearer than this!



Proven Clinical Performance

Despite their delicate appearance, the design and materials that compose Mirage™ ceramic brackets provide unsurpassed strength that is equal to or greater than monocrystal Sapphire brackets. In fact, one of the features that doctors love about the Mirage™ bracket system is that its double fracture toughness (as compared to Sapphire material) increases reliability and decreases chair time.

Unlike Sapphire brackets, the 99.9 percent pure polycrystalline alumina oxide from which Mirage™ brackets are constructed is glare free and completely disguisable on the tooth. It also offers 45 percent less friction as compared to typical saw-cut style Sapphire brackets for faster teeth movement and shorter treatment time.

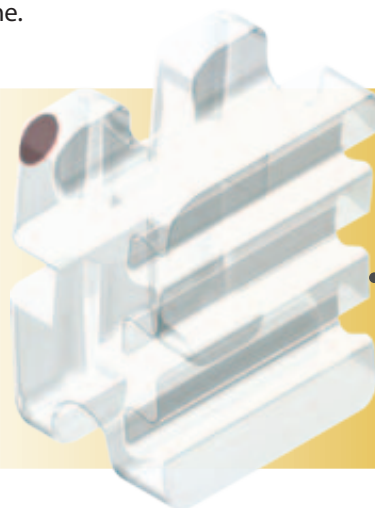

Mechanical Base Bonding for Aesthetics You Can Depend On.

Complementing the sheer strength of the Mirage™ ceramic brackets is a distinctively designed, state-of-the-art mushroom mechanical lock base design that provides excellent adhesion by expanding the surface area between the bracket and the tooth.


Designed with a porous coating that provides millions of additional undercuts that firmly grip the adhesive, Mirage™ brackets feature superior retention and easy debonding characteristics. Additional primer agents are not required to bond Mirage™ brackets to the tooth's enamel. In fact, successful bonding and debonding can be achieved using currently available bonding techniques.

MirageTM


CERAMIC BRACKET SYSTEM

by Orthodontic Design and Production, Inc.

Cosmetic Brackets

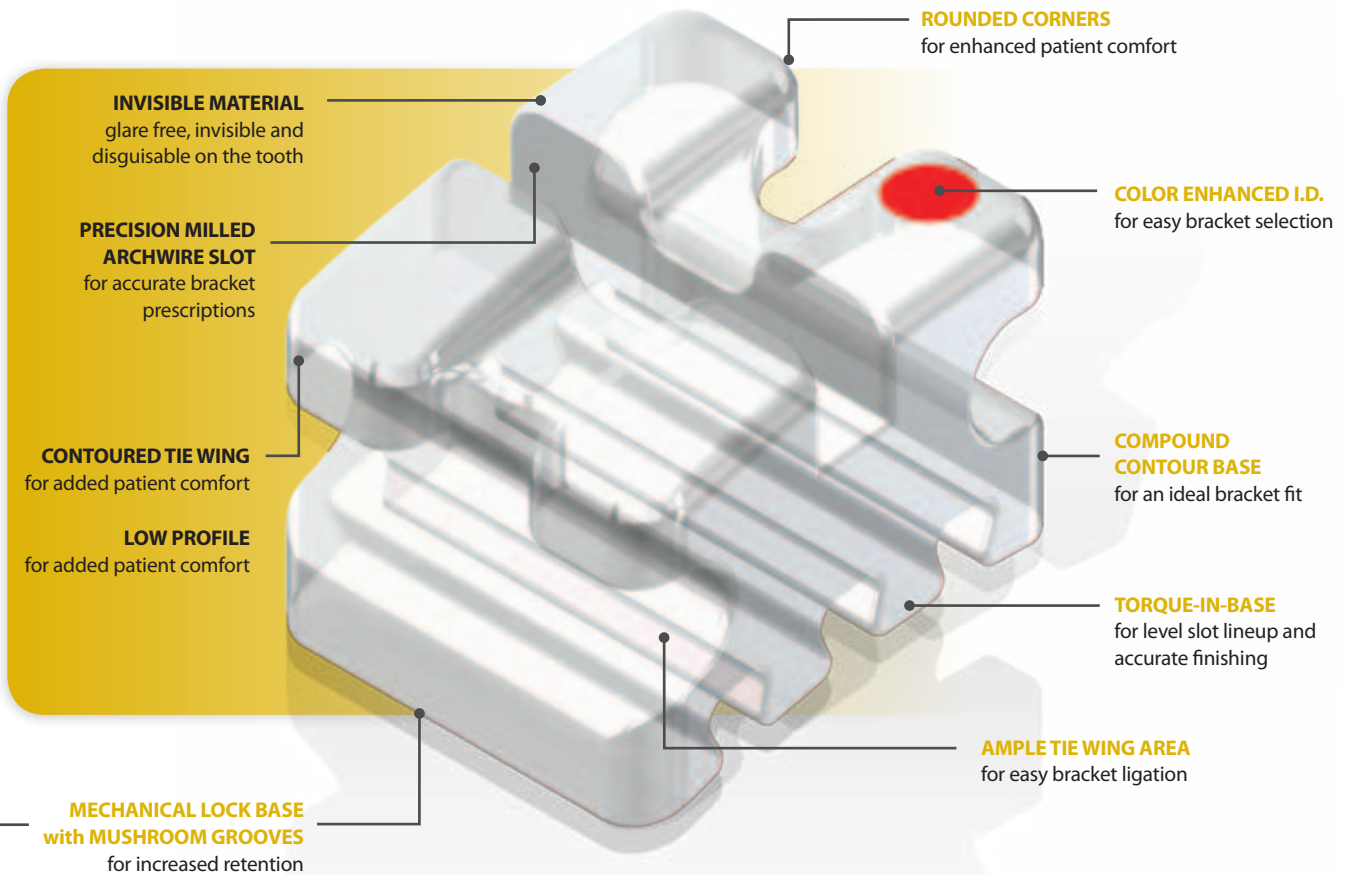

IDENTIFICATION SYSTEM

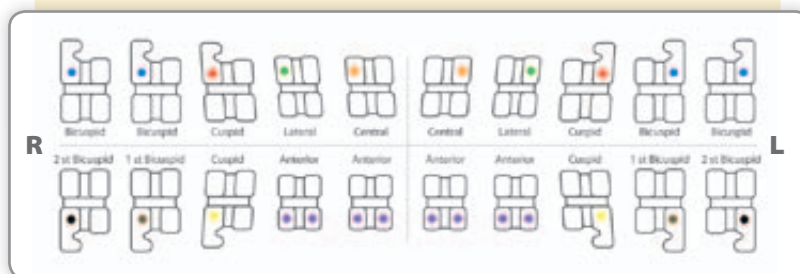

MIRAGE™ CERAMIC BRACKET SYSTEM

Roth[†] Prescription

Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022				
Central	+12°	+5°	0°	3.0 mm	R	●	60-U1-8R	60-U1-2R				
					L	●	60-U1-8L	60-U1-2L				
Lateral	+8°	+9°	0°	3.0 mm	R	●	60-U2-8R	60-U2-2R				
					L	●	60-U2-8L	60-U2-2L				
Cuspid	0°	+11°	+4°	3.0 mm	R	●	60-U3-8R	60-U3-2R				
					L	●	60-U3-8L	60-U3-2L				
Cuspid Hk					R	●	60-U3-8RK	60-U3-2RK				
					L	●	60-U3-8LK	60-U3-2LK				
1 st & 2 nd Bicuspid	-7	0°	0°	3.2 mm	U	●●	60-U4-8U	60-U4-2U				
1 st & 2 nd Bicuspid Hk					R	●	60-U4-8RK	60-U4-2RK				
					L	●	60-U4-8LK	60-U4-2LK				

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	0°	0°	0°	3.0 mm	U	●●	60-L1-8U	60-L1-2U
Cuspid	-11°	+5°	+2°	3.0 mm	R	●	60-L3-8R	60-L3-2R
					L	●	60-L3-8L	60-L3-2L
Cuspid Hk					R	●	60-L3-8RK	60-L3-2RK
					L	●	60-L3-8LK	60-L3-2LK
1 st Bicuspid	-17°	0°	0°	3.2 mm	U	●●	60-L4-8U	60-L4-2U
1 st Bicuspid Hk					R	●	60-L4-8RK	60-L4-2RK
					L	●	60-L4-8LK	60-L4-2LK
2 nd Bicuspid	-22°	0°	0°	3.2 mm	U	●●	60-L5-8U	60-L5-2U
2 nd Bicuspid Hk					R	●	60-L5-8RK	60-L5-2RK
					L	●	60-L5-8LK	60-L5-2LK

Full Sets	.018	.022
Upper/Lower 5X5 No Hooks	60K-NHK-18	60K-NHK-22
Upper/Lower 5X5 No Hook on 3	60K-3-18	60K-3-22
Upper/Lower 5X5 No Hooks on 3, 4, & 5	60K-345-18	60K-345-22

Edgewise Prescription

Maxillary & Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	0°	0°	0°	3.0 mm	U	---	62-CENT-18	62-CENT-22
Lateral	0°	0°	0°	3.0 mm	U	---	62-LAT-18	62-LAT-22
Cuspid	0°	0°	0°	3.0 mm	U	---	62-CUSP-18	62-CUSP-22
Bicuspid	0°	0°	0°	3.2 mm	U	---	62-BIC-18	62-BIC-22
Lower Anterior	0°	0°	0°	3.0 mm	U	---	62-ANT-18	62-ANT-22

Full Sets	.018	.022
Upper/Lower 5x5 No Hooks	62K-EDGE-18	62K-EDGE-22

Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

† ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

MIRAGE™ CERAMIC BRACKET SYSTEM

MBT[†] Prescription

Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	+17°	+4°	0°	3.0 mm	R	●	61-U1-8R	61-U1-2R
					L	●	61-U1-8L	61-U1-2L
Lateral	+10°	+8°	0°	3.0 mm	R	●	61-U2-8R	61-U2-2R
					L	●	61-U2-8L	61-U2-2L
Cuspid	-7°	+8°	0°	3.0 mm	R	●	61-U3-8R	61-U3-2R
					L	●	61-U3-8L	61-U3-2L
Cuspid Hk	0°	+8°	0°	3.0 mm	R	●	61-U3-8RK	61-U3-2RK
					L	●	61-U3-8LK	61-U3-2LK
1 st & 2 nd Bicuspids	-7°	0°	0°	3.2 mm	U	●●	61-U4-8U	61-U4-2U
1 st & 2 nd Bicuspids Hk					R	●	61-U4-8RK	61-U4-2RK
					L	●	61-U4-8LK	61-U4-2LK

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	-6°	0°	0°	3.0 mm	U	●●	61-L1-8U	61-L1-2U
Cuspid	-6°	+3°	0°	3.0 mm	R	●	61-L3-8R	61-L3-2R
					L	●	61-L3-8L	61-L3-2L
Cuspid Hk	0°	+3°	0°	3.0 mm	R	●	61-L3-8RK	61-L3-2RK
					L	●	61-L3-8LK	61-L3-2LK
1 st Bicuspids	-12°	0°	0°	3.2 mm	U	●●	61-L4-8U	61-L4-2U
1 st Bicuspids Hk					R	●	61-L4-8RK	61-L4-2RK
					L	●	61-L4-8LK	61-L4-2LK
2 nd Bicuspids	-17°	0°	0°	3.2 mm	U	●●	61-L5-8U	61-L5-2U
2 nd Bicuspids Hk					R	●	61-L5-8RK	61-L5-2RK
					L	●	61-L5-8LK	61-L5-2LK

Full Sets	.018	.022
Upper/Lower 5x5 No Hooks	61K-NHK-18	61K-NHK-22
Upper/Lower 5x5 Hook on 3	61K-3-18	61K-3-22
Upper/Lower 5x5 Hooks on 3, 4, & 5	61K-345-18	61K-345-22



Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

† ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

Cuspids with 0° torque come standard in kits. Please specify when ordering if you require alternate torque.

Cosmetic Brackets

Beautifully Functional


ODP's comfortable, aesthetically appealing Clarion™ ceramic brackets feature a nickel-free silver alloy-lined archwire slot, making them a safe alternative for nickel-sensitive patients. The metal slot is precisely integrated into the bracket body, creating an eye-pleasing device that offers the sliding mechanics of a metal slot.



Proven Clinical Performance

Doctors love the fact that the design and materials that compose Clarion™ ceramic brackets provide unsurpassed strength, making breakage a thing of the past. The Clarion™ ceramic bracket system also features a unique state-of-the-art dovetail base design for maximum bonding surface between the bracket and the adhesive. The dovetail base provides excellent adhesion by expanding the surface area of the bracket to the tooth. Successful bonding and debonding can be achieved using currently available bonding techniques.

Available in Roth, MBT, and Standard Edgewise prescriptions, Clarion™ ceramic brackets offer the pleasing aesthetics and comfort desired by patients, along with the clinical functionality demanded by doctors.

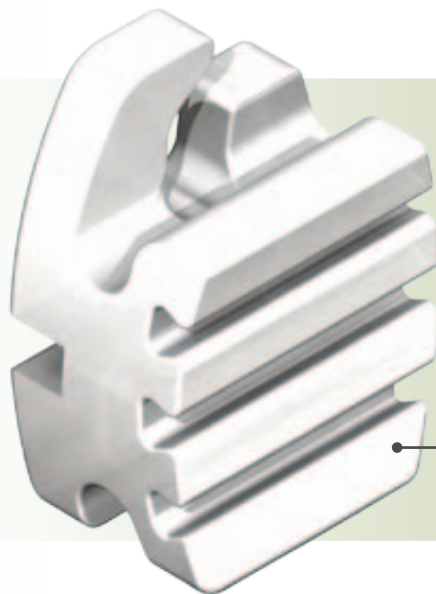

The Preferred Aesthetic Choice

ODP's Clarion™ brackets feature a distinctively designed dove-tailed base for increased surface contact, allowing for excellent adhesion.



The brackets are designed with a porous coating that provides millions of additional undercuts that firmly grip the adhesive. As a result, additional primer agents are not required to bond Clarion™ brackets to the tooth's enamel.

Clarion™ brackets feature superior retention and easy debonding characteristics.

Clarion™

METAL-LINED CERAMIC BRACKET SYSTEM

by Orthodontic Design and Production, Inc.

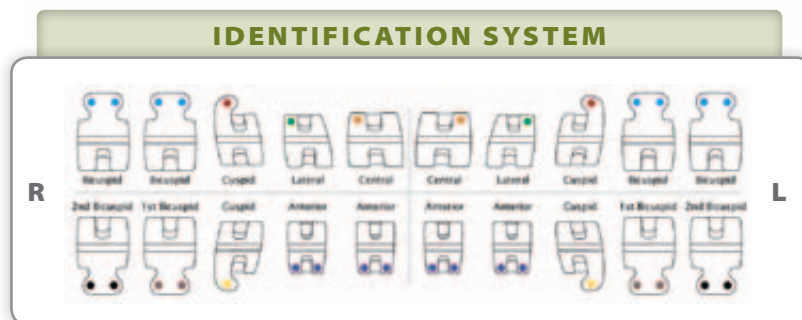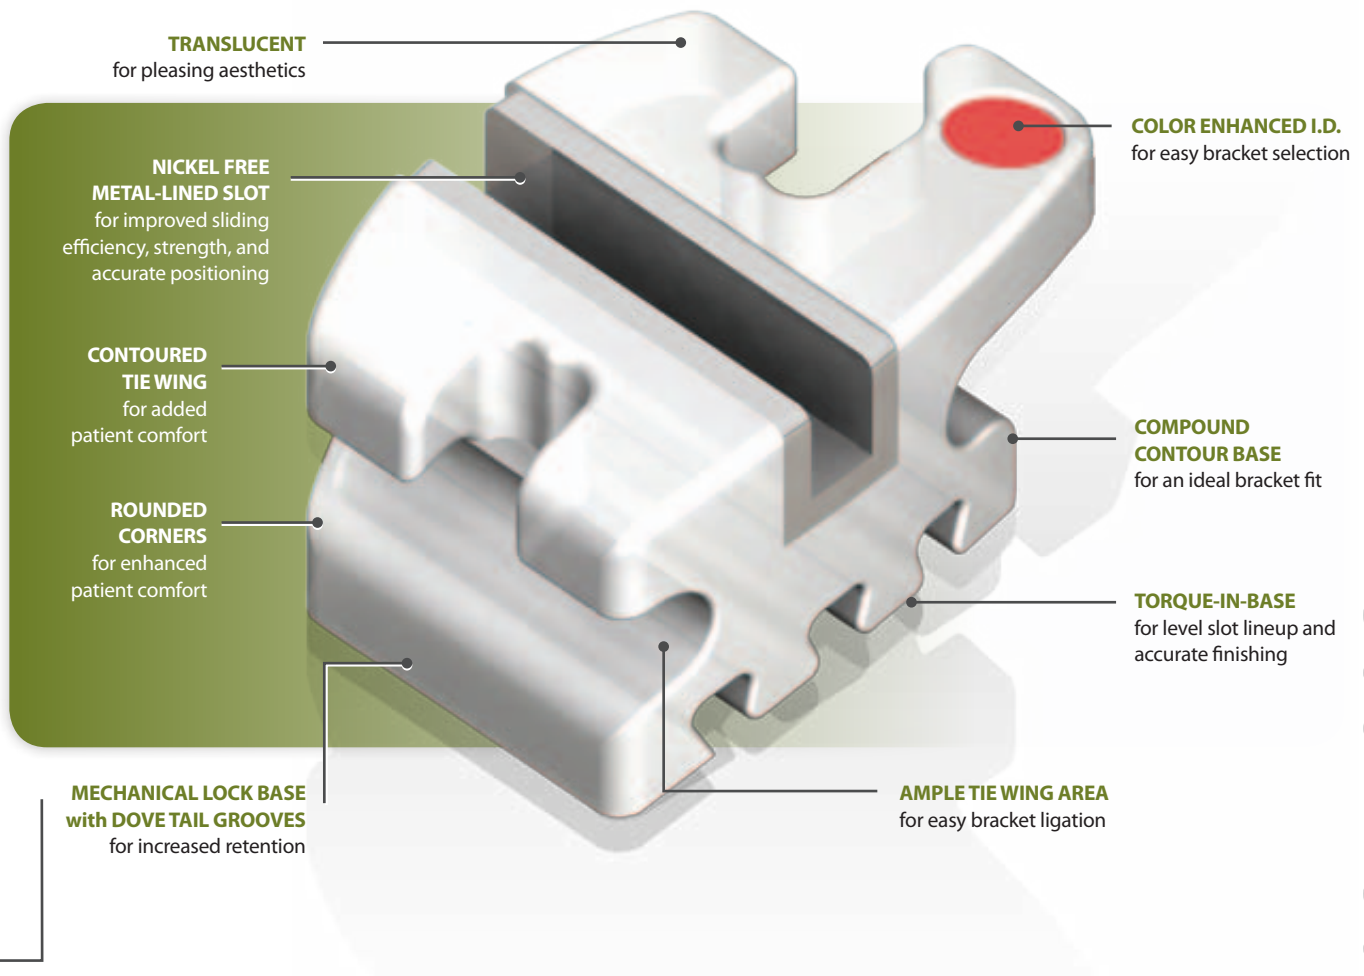

Cosmetic Brackets

CLARION™ METAL-LINED CERAMIC BRACKET SYSTEM

Roth[†] Prescription

Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	+12°	+5°	0°	3.9 mm	R	●	50-U1-8R	50-U1-2R
					L	●	50-U1-8L	50-U1-2L
Lateral	+8°	+9°	0°	3.3 mm	R	●	50-U2-8R	50-U2-2R
					L	●	50-U2-8L	50-U2-2L
Cuspid	0°	+11°	+4°	3.3 mm	R	●	50-U3-8R	50-U3-2R
					L	●	50-U3-8L	50-U3-2L
Cuspid Hk					R	●	50-U3-8RK	50-U3-2RK
					L	●	50-U3-8LK	50-U3-2LK
1 st & 2 nd Bicuspid	-7°	0°	0°	3.3 mm	U	●●	50-U4-8U	50-U4-2U
1 st & 2 nd Bicuspid Hk					U	●●	50-U4-8UK	50-U4-2UK

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	0°	0°	0°	2.8 mm	U	●●	50-L1-8U	50-L1-2U
Cuspid	-11°	+5°	+2°	3.3 mm	R	●	50-L3-8R	50-L3-2R
					L	●	50-L3-8L	50-L3-2L
Cuspid Hk					R	●	50-L3-8RK	50-L3-2RK
					L	●	50-L3-8LK	50-L3-2LK
1 st Bicuspid	-17°	0°	0°	3.3 mm	U	●●	50-L4-8U	50-L4-2U
1 st Bicuspid Hk					U	●●	50-L4-8UK	50-L4-2UK
2 nd Bicuspid	-22°	0°	0°	3.3 mm	U	●●	50-L5-8U	50-L5-2U
2 nd Bicuspid Hk					U	●●	50-L5-8UK	50-L5-2UK

Full Sets	.018	.022
Upper/Lower 5X5 No Hooks	50K-NHK-18	50K-NHK-22
Upper/Lower 5X5 No Hook on 3	50K-3-18	50K-3-22
Upper/Lower 5X5 No Hooks on 3, 4, & 5	50K-345-18	50K-345-22

Edgewise Prescription

Maxillary & Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	0°	0°	0°	3.9 mm	U	---	52-CENT-18	52-CENT-22
Lateral	0°	0°	0°	3.3 mm	U	---	52-LAT-18	52-LAT-22
Cuspid	0°	0°	0°	3.3 mm	U	---	52-CUSP-18	52-CUSP-22
Bicuspid	0°	0°	0°	3.3 mm	U	---	52-BIC-18	52-BIC-22
Lower Anterior	0°	0°	0°	2.8 mm	U	---	52-ANT-18	52-ANT-22

Full Sets	.018	.022
Upper/Lower 5x5 No Hooks	52K-EDGE-18	52K-EDGE-22

Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

† ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

CLARION™ METAL-LINED CERAMIC BRACKET SYSTEM
MBT[†] Prescription
Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	+17°	+4°	0°	3.9 mm	R	●	51-U1-8R	51-U1-2R
					L	●	51-U1-8L	51-U1-2L
Lateral	+10°	+8°	0°	3.3 mm	R	●	51-U2-8R	51-U2-2R
					L	●	51-U2-8L	51-U2-2L
Cuspid	-7°	+8°	0°	3.3 mm	R	●	51-U3-8R	51-U3-2R
					L	●	51-U3-8L	51-U3-2L
Cuspid Hk	0°	+8°	0°	3.3 mm	R	●	51-U3-8RK	51-U3-2RK
					L	●	51-U3-8LK	51-U3-2LK
1 st & 2 nd Bicuspid	-7°	0°	0°	3.3 mm	U	●●	51-U4-8U	51-U4-2U
1 st & 2 nd Bicuspid Hk					U	●●	51-U4-8UK	51-U4-2UK

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	-6°	0°	0°	2.8 mm	U	●●	51-L1-8U	51-L1-2U
Cuspid	-6°	+3°	0°	3.3 mm	R	●	51-L3-8R	51-L3-2R
					L	●	51-L3-8L	51-L3-2L
Cuspid Hk	0°	+3°	0°	3.3 mm	R	●	51-L3-8RK	51-L3-2RK
					L	●	51-L3-8LK	51-L3-2LK
1 st Bicuspid	-12°	+2°	0°	3.3 mm	R	●	51-L4-8R	51-L4-2R
					L	●	51-L4-8L	51-L4-2L
1 st Bicuspid Hk					R	●	51-L4-8RK	51-L4-2RK
					L	●	51-L4-8LK	51-L4-2LK
2 nd Bicuspid	-17°	+2°	0°	3.3 mm	R	●	51-L5-8R	51-L5-2R
					L	●	51-L5-8L	51-L5-2L
2 nd Bicuspid Hk					R	●	51-L5-8RK	51-L5-2RK
					L	●	51-L5-8LK	51-L5-2LK

Full Sets	.018	.022
Upper/Lower 5x5 No Hooks	51K-NHK-18	51K-NHK-22
Upper/Lower 5x5 Hook on 3	51K-3-18	51K-3-22
Upper/Lower 5x5 Hooks on 3, 4, & 5	51K-345-18	51K-345-22



Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

[†] ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

Cuspids with 0° torque come standard in kits. Please specify when ordering if you require alternate torque.

Cosmetic Brackets

The Preferred Aesthetic Choice


Your patients will be thrilled with the transparent aesthetic appearance of Diamante™ ceramic brackets. Not only are Diamante™ ceramic brackets nearly invisible, but the 99.9 percent pure polycrystalline alumina from which they are composed is impervious to stains and discolorations, helping them stay transparent for the duration of the treatment. In addition to their coveted aesthetic qualities, Diamante™ ceramic brackets are small and smooth, with rounded corners that provide a comfort level surpassed by none.



Proven Clinical Performance

Doctors love the fact that the design and materials that compose Diamante™ ceramic brackets provide unsurpassed strength, making breakage a thing of the past. The Diamante™ ceramic bracket system also features a unique state-of-the-art dovetail base design for maximum bonding surface between the bracket and the adhesive. The dovetail base provides excellent adhesion by expanding the surface area of the bracket to the tooth. Successful bonding and debonding can be achieved using currently available bonding techniques.

Available in Roth, Roth V-Slot (.025 x .025), MBT, and Standard Edge-wise prescriptions, Diamante™ ceramic brackets offer the pleasing aesthetics and comfort desired by patients, along with the clinical functionality demanded by doctors.

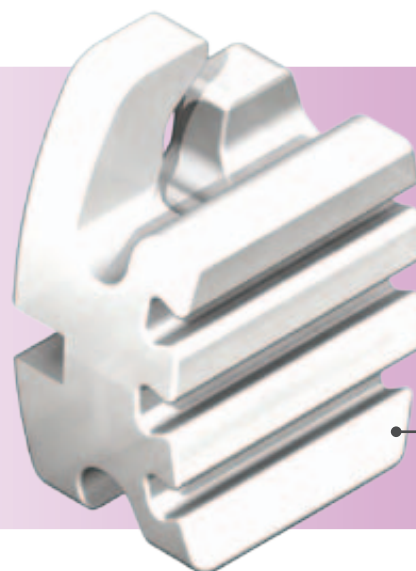

Innovation, from the Bottom Up



ODP's Diamante™ brackets feature a distinctively designed dovetailed base for increased surface contact, allowing for excellent adhesion.

The brackets are designed with a porous coating that provides millions of additional undercuts that firmly grip the adhesive. As a result, additional primer agents are not required to bond Diamante™ brackets to the tooth's enamel.

Diamante™ brackets feature superior retention and easy debonding characteristics.

Diamante™ CERAMIC BRACKET SYSTEM

by Orthodontic Design and Production, Inc.

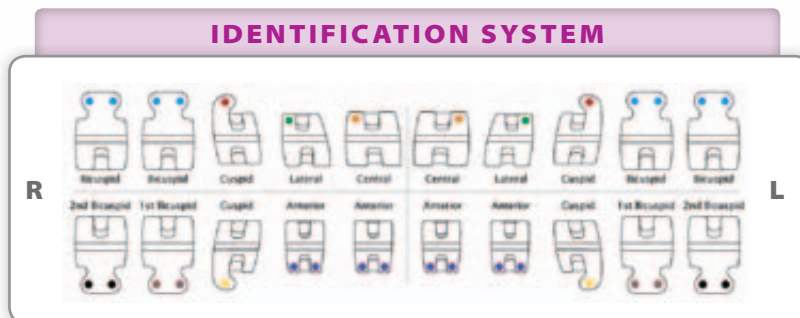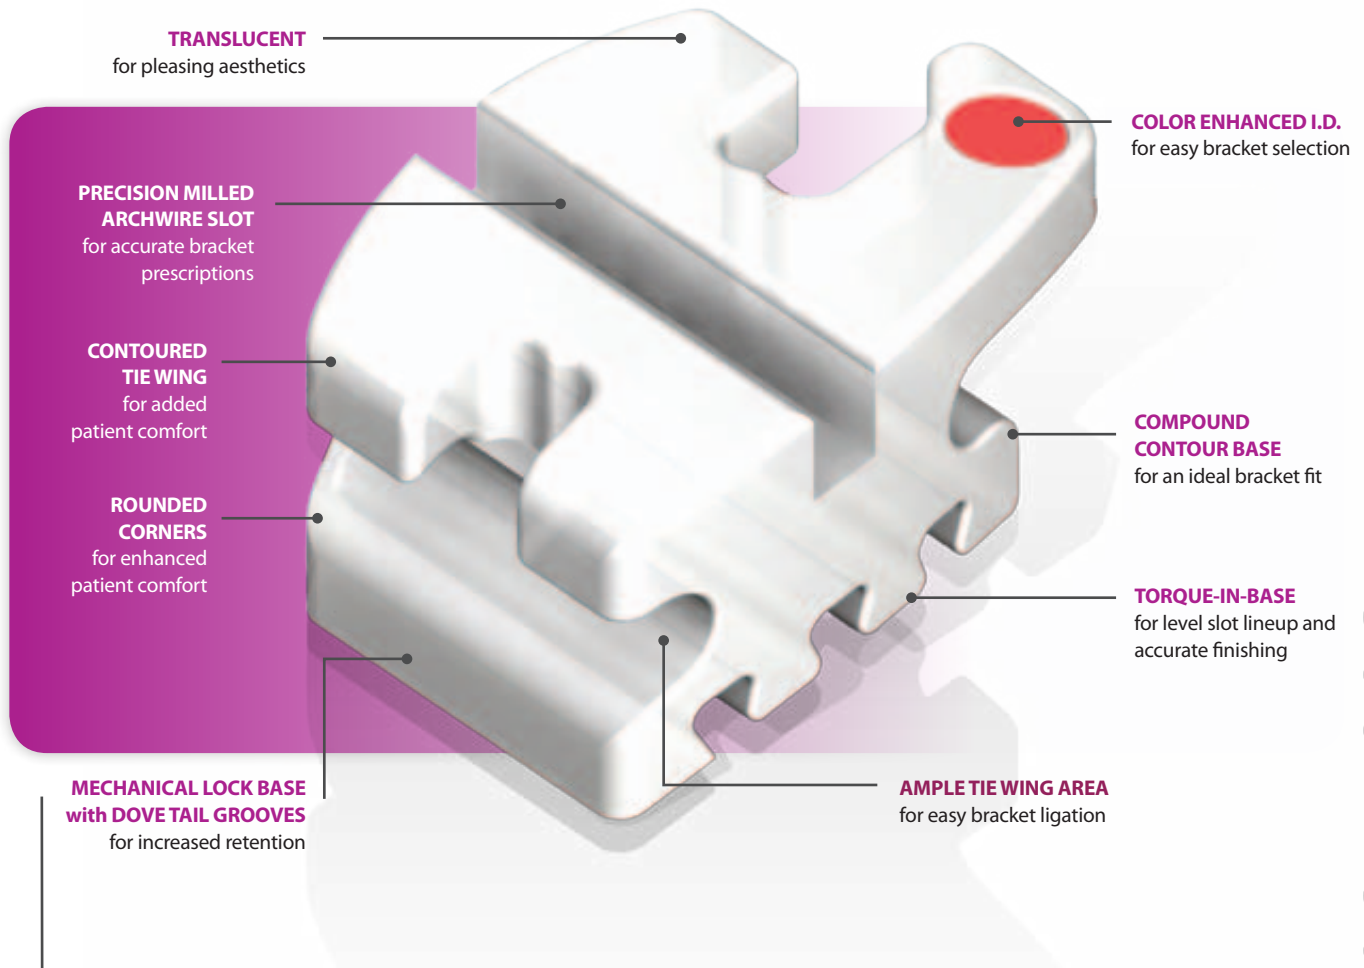

Cosmetic Brackets

DIAMANTE™ CERAMIC BRACKET SYSTEM

Roth[†] Prescription

Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	+12°	+5°	0°	3.9 mm	R	●	55-U1-8R	55-U1-2R
					L	●	55-U1-8L	55-U1-2L
Lateral	+8°	+9°	0°	3.3 mm	R	●	55-U2-8R	55-U2-2R
					L	●	55-U2-8L	55-U2-2L
Cuspid	0°	+11°	+4°	3.3 mm	R	●	55-U3-8R	55-U3-2R
					L	●	55-U3-8L	55-U3-2L
Cuspid Hk					R	●	55-U3-8RK	55-U3-2RK
					L	●	55-U3-8LK	55-U3-2LK
1 st & 2 nd Bicuspid	-7°	0°	0°	3.3 mm	U	●●	55-U4-8U	55-U4-2U
1 st & 2 nd Bicuspid Hk					U	●●	55-U4-8UK	55-U4-2UK

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	0°	0°	0°	2.8 mm	U	●●	55-L1-8U	55-L1-2U
Cuspid	-11°	+5°	+2°	3.3 mm	R	●	55-L3-8R	55-L3-2R
					L	●	55-L3-8L	55-L3-2L
Cuspid Hk					R	●	55-L3-8RK	55-L3-2RK
					L	●	55-L3-8LK	55-L3-2LK
1 st Bicuspid	-17°	0°	0°	3.3 mm	U	●●	55-L4-8U	55-L4-2U
1 st Bicuspid Hk					U	●●	55-L4-8UK	55-L4-2UK
2 nd Bicuspid	-22°	0°	0°	3.3 mm	U	●●	55-L5-8U	55-L5-2U
2 nd Bicuspid Hk					U	●●	55-L5-8UK	55-L5-2UK

Full Sets	.018	.022
Upper/Lower 5X5 No Hooks	55K-NHK-18	55K-NHK-22
Upper/Lower 5X5 No Hook on 3	55K-3-18	55K-3-22
Upper/Lower 5X5 No Hooks on 3, 4, & 5	55K-345-18	55K-345-22

Edgewise Prescription

Maxillary & Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	0°	0°	0°	3.9 mm	U	---	58-CENT-18	58-CENT-22
Lateral	0°	0°	0°	3.3 mm	U	---	58-LAT-18	58-LAT-22
Cuspid	0°	0°	0°	3.3 mm	U	---	58-CUSP-18	58-CUSP-22
Bicuspid	0°	0°	0°	3.3 mm	U	---	58-BIC-18	58-BIC-22
Lower Anterior	0°	0°	0°	2.8 mm	U	---	58-ANT-18	58-ANT-22

Full Sets	.018	.022
Upper/Lower 5x5 No Hooks	58K-EDGE-18	58K-EDGE-22

Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

[†] ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

DIAMANTE™ CERAMIC BRACKET SYSTEM

Roth† V Slot Prescription

Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	+12°	+5°	0°	3.9 mm	R	●	56-U1-8R	56-U1-2R
					L	●	56-U1-8L	56-U1-2L
Lateral	+8°	+9°	0°	3.3 mm	R	●	56-U2-8R	56-U2-2R
					L	●	56-U2-8L	56-U2-2L
Cuspid	0°	+11°	+4°	3.3 mm	R	●	56-U3-8R	56-U3-2R
					L	●	56-U3-8L	56-U3-2L
Cuspid Hk					R	●	56-U3-8RK	56-U3-2RK
					L	●	56-U3-8LK	56-U3-2LK
1 st & 2 nd Bicuspid	-7°	0°	0°	3.3 mm	U	●●	56-U4-8U	56-U4-2U
1 st & 2 nd Bicuspid Hk					U	●●	56-U4-8UK	56-U4-2UK

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	0°	0°	0°	2.8 mm	U	●●	56-L1-8U	56-L1-2U
Cuspid	-11°	+5°	+2°	3.3 mm	R	●	56-L3-8R	56-L3-2R
					L	●	56-L3-8L	56-L3-2L
Cuspid Hk					R	●	56-L3-8RK	56-L3-2RK
					L	●	56-L3-8LK	56-L3-2LK
1 st Bicuspid	-17°	0°	0°	3.3 mm	U	●●	56-L4-8U	56-L4-2U
1 st Bicuspid Hk					U	●●	56-L4-8UK	56-L4-2UK
2 nd Bicuspid	-22°	0°	0°	3.3 mm	U	●●	56-L5-8U	56-L5-2U
2 nd Bicuspid Hk					U	●●	56-L5-8UK	56-L5-2UK

Full Sets	.018	.022
Upper/Lower 5X5 No Hooks	56K-NHK-18	56K-NHK-22
Upper/Lower 5X5 No Hook on 3	56K-3-18	56K-3-22
Upper/Lower 5X5 No Hooks on 3, 4, & 5	56K-345-18	56K-345-22



Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

† ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

Cosmetic Brackets

DIAMANTE™ CERAMIC BRACKET SYSTEM

MBT[†] Prescription

Maxillary

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Central	+17°	+4°	0°	.137"	R	●	57-U1-8R	57-U1-2R
					L	●	57-U1-8L	57-U1-2L
Lateral	+10°	+8°	0°	.118"	R	●	57-U2-8R	57-U2-2R
					L	●	57-U2-8L	57-U2-2L
Cuspid	-7°	+8°	0°	.137"	R	●	57-U3-8R	57-U3-2R
					L	●	57-U3-8L	57-U3-2L
Cuspid Hk	0°	+8°	0°	.137"	R	●	57-U3-8RK	57-U3-2RK
					L	●	57-U3-8LK	57-U3-2LK
1 st & 2 nd Bicuspid	-7°	0°	0°	.118"	U	●●	57-U4-8U	57-U4-2U
1 st & 2 nd Bicuspid Hk					U	●●	57-U4-8UK	57-U4-2UK

Mandibular

Tooth	Torque	Angle	Rotation	M/D	R/L	ID	.018	.022
Anterior	-6°	0°	0°	.100"	U	●●	57-L1-8U	57-L1-2U
Cuspid	-6°	+3°	0°	.122"	R	●	57-L3-8R	57-L3-2R
					L	●	57-L3-8L	57-L3-2L
Cuspid Hk	0°	+3°	0°	.122"	R	●	57-L3-8RK	57-L3-2RK
					L	●	57-L3-8LK	57-L3-2LK
1 st Bicuspid	-12°	+2°	0°	.120"	R	●	57-L4-8R	57-L4-2R
					L	●	57-L4-8L	57-L4-2L
1 st Bicuspid Hk					R	●	57-L4-8RK	57-L4-2RK
					L	●	57-L4-8LK	57-L4-2LK
2 nd Bicuspid	-17°	+2°	0°	.120"	R	●	57-L5-8R	57-L5-2R
					L	●	57-L5-8L	57-L5-2L
2 nd Bicuspid Hk					R	●	57-L5-8RK	57-L5-2RK
					L	●	57-L5-8LK	57-L5-2LK

Full Sets	.018	.022
Upper/Lower 5x5 No Hooks	57K-NHK-18	57K-NHK-22
Upper/Lower 5x5 Hook on 3	57K-3-18	57K-3-22
Upper/Lower 5x5 Hooks on 3, 4, & 5	57K-345-18	57K-345-22

Also available in pre-packaged single case kits for your convenience.

Please add an -01 to the end of the kit part number (see Full Sets section). Contact us for pricing and quantity requirements.

[†] ODP prescriptions are not implied to be an exact version of any other system, nor do we claim any endorsement by the doctor.

Cuspid with 0° torque come standard in kits. Please specify when ordering if you require alternate torque.

Bracket Organizers

In today's market, you have to stand out, and customization provides a great way to market your brand. Packaging should achieve a balance of image, practicality and performance. ODP now offers unique, very stylish bracket organizers. They allow for each bracket type to be stored in a separate compartment for ease of inventory. This feature also prevents cross-contamination, which is ideal for today's strict OSHA regulations.

Upon request, we will pre-pack individual cases for your convenience. Contact us for pricing and quantity requirements.

Plain without artwork	M604-00
Comfort Zone™	M604-01
Comfort Zone Hybrid™	M604-02
Magnum™	M604-03
Lucent™	M604-04
Prism™	M604-05
Clarion™	M604-06
Diamante™	M604-07
Cannon Ultra™	M604-08
Cannon Ultra II™	M604-09
Focus™	M604-10
Agility®	M604-11
Mirage™	M604-12
Discreet™	M604-13



Circular Bracket Organizers

ODP's convenient, compact circular bracket organizers are ideal for chairside bonding procedures. The clear rotating lid allows for easy retrieval of the desired bracket. Upon request, we will pre-pack individual cases for your convenience.



Holds up to 25 cases

ORDER NUMBER M600-01



Holds individual cases

ORDER NUMBER M605-01

Cosmetic Brackets